


Lab Notebook Entry from LeCroy DSO
DSO S/N: LCRY2805N56957
User: HSHL-User
Time: 12.01.2026 18:50:19

Report--00001



LabNotebook

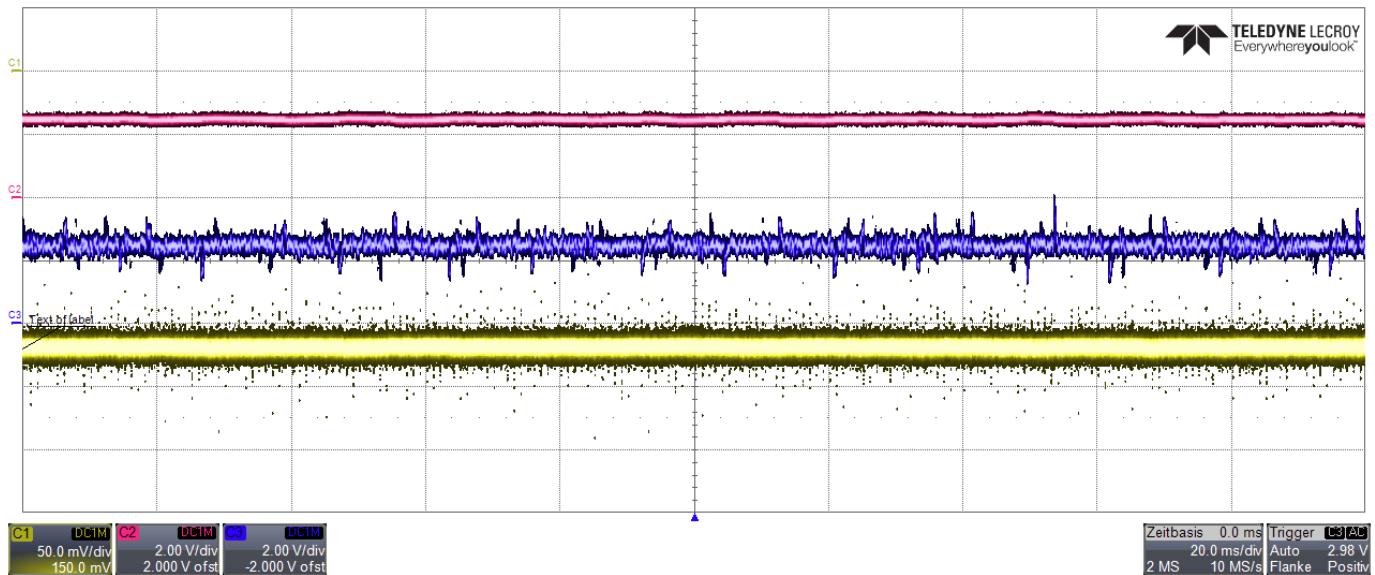

Channel Status

	C1	C2	C3
V / Div	50.0 mV	2.00 V	2.00 V
Offset	150.0 mV	2.000 V	-2.000 V
Coupling	DC1MΩ	DC1MΩ	DC1MΩ
BW-Limit	1GHZ	1GHZ	1GHZ
Probe	10.0000	10	10.0000
Sweeps	1 #	1 #	1 #

Acquisition Status

	Time / Div	20.0 ms	Sampling Rate	10.000000 MS/s
Horizontal	Time / Pt	100.000000 ns	Sampling Mode	RealTime
	Pts / Div	200.0000 kS	Trigger Delay	0.0 ms
	Mode	Auto	Slope	Positive
Trigger	Type	Edge	Level	2.98 V
	Source	C3	Coupling	AC